




ENDO 6:1










English

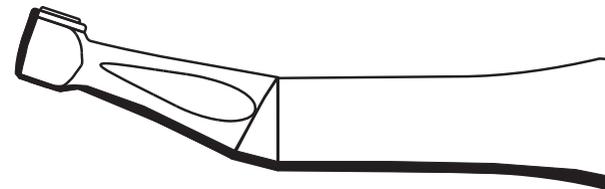

Operating Instructions



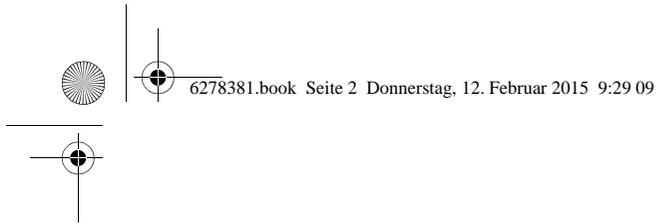



Operating Instructions ENDO 6:1

Table of contents



Table of contents

1	Before you begin	6
1.1	Structure of the document	7
1.2	Service life of Sirona instruments	10
2	Safety information	11
3	Technical description	13
3.1	Task	13
3.2	ENDO 6:1 components	13
3.3	Technical data	14
4	Preparation	18
4.1	Initial start-up and longer breaks in use	18



62 78 381 D3451.201.01.05.02









Table of contents

Operating Instructions ENDO 6:1



5	Operation	19
5.1	Replacing the instrument.....	19
5.2	Attaching and removing a file	21
5.3	Recommendation for the treatment procedure.....	22
5.4	Mounting and removing the insulating sleeve	24
6	Follow-up	26
6.1	After each treatment session.....	26
6.2	At the end of the work day.....	27







Operating Instructions ENDO 6:1

Table of contents

7	Conditioning	28
7.1	Conduct pre-disinfection.....	28
7.2	Automated cleaning and disinfecting	29
7.3	Manual cleaning and disinfection	32
7.4	Manual maintenance	34
7.5	Sterilizing.....	37
8	Spare parts and consumables	39
9	Storage and transport conditions	40
10	Disposal	41





1 Before you begin ...

Intended use



Contraindications

Target group

6



Operating Instructions ENDO 6:1

1 Before you begin ...

ENDO 6:1 is used to hold and drive burr instruments for the purposes of rotary processing and is intended for the following uses in dentistry:

- Endodontics
- Endometry

ENDO 6:1 complies state-of-the-art technical regulations. ENDO 6:1 complies with the ISO 14457 standard.

1. Read the operating instructions prior to using ENDO 6:1.
2. Only use ENDO 6:1 for the applications described in the operating instructions.
3. Observe the applicable hygiene standards, occupational safety regulations and accident prevention measures for ENDO 6:1.

None

This product is intended only for use by trained dental personnel in dental practices and laboratories.

62 78 381 D3451.201.01.05.02





Warnings



Instructions for use



1.1 Structure of the document

1.1.1 Labeling of information

➤ To prevent injuries, please observe all warnings.

Warnings are labeled as follows:

⚠ DANGER! indicates a danger **leading** to death or serious injury if not avoided.


⚠ WARNING! indicates a danger that **may lead** to death or serious injury if not avoided.

⚠ CAUTION! indicates a danger that **may lead** to injury if not avoided.

➤ To prevent material damage and additional expenses, please observe all instructions for use.

Instructions for use are labeled as follows:

NOTICE! indicates measures for the prevention of material damage.







1 Before you begin ...




8





Operating Instructions ENDO 6:1



62 78 381 D3451.201.01.05.02





1.1.2 Formats and symbols

The formats and symbols used in this document have the following meaning:

✓ Prerequisite	Requests you to do something.
1. First action step	
2. Second action step	
or	
> Alternative action	
⚡ Result	
➤ Individual action step	



1 Before you begin ...

Operating Instructions ENDO 6:1



Use of formats and symbols [→ 9].	Identifies a reference to another text passage and specifies its page number.
• List	Identifies a list.



1.2 Service life of Sirona instruments

When used as intended:


- Non-moving parts of Sirona instruments have a typical service life of approx. 5 years
- Moving parts of Sirona instruments have a typical service life of approx. 3 years

No warranty claim can be inferred here, as wear may occur earlier or later than indicated above depending on use, frequency of sterilization, and frequency of maintenance.



10

62 78 381 D3451.201.01.05.02





Obligations of the user

2 Safety information

- Use only fault-free materials that do **not** deviate from the specified data [→ 14].
- Protect yourself, patients, and others against any foreseeable dangers. To do this, follow the safety information.
- Comply with the Intended use of the equipment.
- You should always keep these operating instructions within reach for further reference.



Preventing the spread of infections and cross contamination


Prevent the spread of infections and cross contamination between patients, users, and third parties. Sterilize equipment after each patient.




Instrument head overheating

Take the appropriate hygiene measures, e.g. wear protective gloves.

If the instrument is defective, the area around the instrument head may heat up, thus creating a risk of burning the patient's oral mucosa.





2 Safety information

Operating Instructions ENDO 6:1



Malfunction or damage

Discontinue use immediately in case of malfunction or damage. Damaged instruments may cause injury. Notify the dental depot or the manufacturer.

Repair


Do **not** repair the instrument yourself.




Spare and accessory parts

Use only original Sirona parts or parts approved by Sirona. Safe operation is **not** guaranteed for parts that have not been approved by Sirona.



If you have any questions, please contact your dental depot or the manufacturer.






3 Technical description

3.1 Task

The instrument serves for transmitting the driving power and speed of the electric motor or air motor (handpiece coupling according to ISO 3964) to the preparation tool.





3.2 ENDO 6:1 components

Contra-angle handpiece

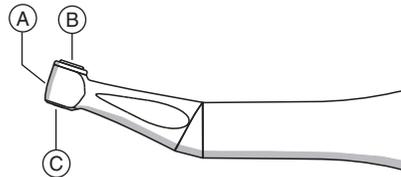


62 78 381 D3451.201.01.05.02

A	Instrument head
B	Pushbutton
C	Opening for the clamping system



3 Technical description

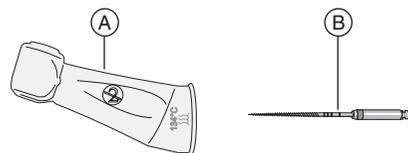

Operating Instructions ENDO 6:1


Accessories

A	Insulating sleeve
B	File



3.3 Technical data
Instrument


	ENDO 6:1
Gear ratio	6:1
Maximum motor speed in rpm	40 000

62 78 381 D3451.201.01.05.02



	ENDO 6:1
Maximum operating speed in rpm	6 700
Clamping system	CA
Internal cooling media	-
Back suction stop	-
Light function	-
Apex measuring function ¹	x
Instrument coupling	INTRAmatic®





3 Technical description

Operating Instructions ENDO 6:1




File

	ENDO 6:1
Shank diameter in mm	2.334 - 2.35
Maximum total length in mm	25
Maximum working diameter in mm (ISO 2157)	2.1
Standard	ISO 1797-1


Coupling

	ENDO 6:1
Standard	ISO 3964



16

62 78 381 D3451.201.01.05.02







Treatment center




	ENDO 6:1
Spray air pressure in bar	2.7
Spray water pressure in bar	2.0
Maximum water temperature in °C	40
Recommended water content in spray in ml/min	> 50

This product bears the CE marking in accordance with the provisions of Council Directive 93/42/EEC of June 14, 1993 concerning medical devices.



CE
0123








4 Preparation

4.1 Initial start-up and longer breaks in use

- Sterilize the instrument and accessories prior to startup.
- Clean and maintain the instrument after longer breaks in use.



5 Operation

NOTICE! Use only faultless files in order to prevent fatigue fractures of the files as far as possible.


⚠ CAUTION! Do not pull the patient's cheek back with the contra-angle handpiece while the motor is running. This would actuate the pushbutton, thus creating a risk of burning the patient's oral mucosa.

5.1 Replacing the instrument

⚠ CAUTION! The instrument should only be fitted or removed when the motor is at standstill.



5 Operation

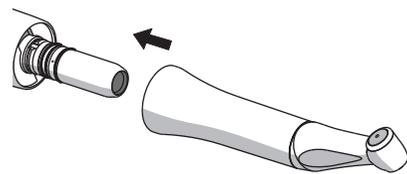




Attaching the ENDO 6:1


- ✓ The motor is at a standstill.
- Insert the instrument until it snaps into place.

Removing the ENDO 6:1

- ✓ The motor is at a standstill.
- Detach the instrument. Do not pull on the supply hose while doing this.

Operating Instructions ENDO 6:1





5.2 Attaching and removing a file

NOTICE! Use only faultless files in order to prevent fatigue fractures of the files as far as possible.

Attaching a file



✓ The drive has come to a stop.



1. Insert the file by gently rotating it until it snaps into place. In doing so, do **not** press the pushbutton.
2. Then pull and turn the file to check that it is firmly seated.

Removing a file

✓ The file has come to a stop.

- Remove it while pressing and holding down the pushbutton.






5.3 Recommendation for the treatment procedure


NOTICE! Use only faultless files in order to prevent fatigue fractures of the files as far as possible.

- The different file systems require different working techniques. For this reason, please always observe the information provided by the file manufacturer.
- Work without exerting any pressure on the file.
- The ApexLocator function is used to support the root canal preparation process in combination with SIROEndo Pocket or a treatment center with the apex measurement function. The number of X-rays can be reduced with ENDO 6:1. However, you must always take at least one X-ray to determine the depth for preparatory work. A clinical evaluation including knowledge of the anatomy of root canals is important for interpreting the results.





Operating Instructions ENDO 6:1

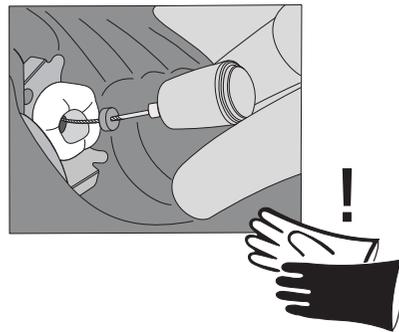

5 Operation

- When performing the APEX measurement, wear appropriate insulated gloves. We recommend performing the treatment with a cofferdam, while using an insulating sleeve. This will prevent inaccurate measurements caused by undesired leakage currents. During the measurement, the instrument must not come into contact with the patient's mucosa, metallic tooth restorations, or the mucosal electrode.
- If the limit torque is exceeded, a gentle creaking may be heard and vibrations felt. Remove the file by gently pulling it toward the coronal end. If this is not possible, switch the drive to counterclockwise rotation and pull the file out of the channel.
IMPORTANT: Check the file afterwards for damage or deformation (untwisting) and replace it, where necessary.





5 Operation

Operating Instructions ENDO 6:1





5.4 Mounting and removing the insulating sleeve

NOTICE! Insulating sleeves are only used once. Change the insulating sleeve after each patient. 

Fitting an insulating sleeve


- ✓ You have sterilized the insulating sleeve.
- ✓ The motor has come to a stop.
- ✓ A file is **not** clamped in place.

1. Twist the insulating sleeve carefully this way and that and pull the insulating sleeve fully over the instrument.
2. Attach the file [→ 21].

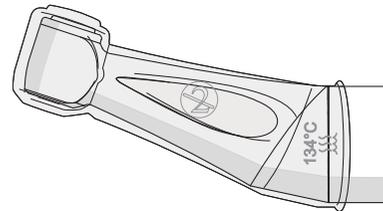

24

62 78 381 D3451.201.01.05.02





6278381.book Seite 25 Donnerstag, 12. Februar 2015 9:29 09




Operating Instructions ENDO 6:1



62 78 381 D3451.201.01.05.02



5 Operation



25





6 Follow-up


6.1 After each treatment session



NOTICE! Condition immediately, or at the latest, one hour after treatment.

NOTICE! Only use Sirona T1 spray.

✓ Wear appropriate protective clothing.

1. Remove the file with tweezers.
2. Pre-disinfect directly at the treatment center/tabletop unit [→ 28].
3. Detach the instrument from the drive.
4. Transport the instrument to the hygiene room in a suitable transport container.
5. Conduct automatic conditioning [→ 29]. Manual conditioning [→ 32] is possible in exceptional cases if the national/local regulations are followed.








- 6. Apply spray to the instrument [→ 34].
- 7. Sterilize the instrument and accessories [→ 37].

6.2 At the end of the work day

NOTICE! Do not leave any instruments on the motor overnight, in order to prevent oil from leaking into the electric motor. Never lubricate the electric motor.



7 Conditioning

7.1 Conduct pre-disinfection



- ✓ Wear appropriate protective clothing.
- ✓ All disinfectants must be approved in your country and have proven bactericidal, fungicidal and virucidal properties. Only use disinfectants with **no** protein-fixing properties.


1. Spray the surface with disinfectant.
2. Wipe the disinfectant off with a cloth.

↪ For further conditioning, the instrument should be dry and free of residue.

In the USA and Canada, for example, you can use:

- CAVICIDE®
- CAVIWIPES™





Please observe the manufacturer's instructions for using instrument disinfectants.





7.2 Automated cleaning and disinfecting ...

7.2.1 ... with a DAC UNIVERSAL

We recommend using **Sirona DAC UNIVERSAL** for automated cleaning, disinfection, care, and unwrapped sterilization.

For further details, refer to the operating instructions supplied with the unit.

- ✓ The pushbutton chuck is manually maintained [→ 35].
 - ✓ The instrument is conditioned using the DAC UNIVERSAL.
1. Check whether the instrument is clean after conditioning under good lighting (min. 500 lux) and color rendering index (min. 80 Ra).
 2. If it is still dirty, repeat the process.





7 Conditioning

Operating Instructions ENDO 6:1

↳ For further conditioning, the instrument should be dry and free of residue.

- 3. Pack the instrument in packaging material suitable for sterilization and storage. e.g. paper/plastic composite packaging.
- 4. Sterilize the instrument [→ 37].

7.2.2 ... with cleaning and disinfection equipment

The instrument can also be cleaned and disinfected in a suitable piece of cleaning and disinfection equipment.


The cleaning and disinfection equipment used must be approved by its manufacturer for the cleaning and disinfection of dental instruments and comply with EN ISO 15883-1 (e.g. 95°C (203°F) and 10 min. holding time).



For further details, refer to the operating instructions supplied with the unit.




30




62 78 381 D3451.201.01.05.02





- ✓ The instrument is conditioned with a cleaning and disinfection device.
- 1. Check whether the instrument is clean after conditioning under good lighting (min. 500 lux) and color rendering index (min. 80 Ra).
- 2. If it is still dirty, repeat the process.
 - ↳ For further conditioning, the instrument should be dry and free of residue.
- 3. Blow the instrument out with max. 3 bar.
- 4. Manual care of mechanical parts [→ 34].
- 5. Manual care of the push button chuck [→ 35].
- 6. Pack the instrument in packaging material suitable for sterilization and storage. e.g. paper/plastic composite packaging.
- 7. Sterilize the instrument [→ 37].





7.3 Manual cleaning and disinfection

NOTICE! Condition immediately, or at the latest, one hour after treatment.



NOTICE! Never clean in an ultrasound bath!


NOTICE! Never immerse in disinfectants!

NOTICE! Only use Sirona T1 spray.



IMPORTANT: Use a soft, clean, and disinfected brush for cleaning.

- ✓ Wear appropriate protective clothing.
 - ✓ All disinfectants must be approved in your country and have proven bactericidal, fungicidal and virucidal properties. Only use disinfectants with **no** protein-fixing properties.
1. Brush the instrument under running water (< 38 °C, < 100 °F, at least drinking water quality) and good lighting (min. 500 lux) and color rendering index (min. 80 Ra) until no more dirt can be seen, for at least 10 seconds.





2. Flush the drive channels with spray.
3. Conduct thermal disinfection or unwrapped steam sterilization.
4. Maintain mechanical parts manually [→ 34].
5. Maintain the push button chuck manually [→ 35].
6. Pack the instrument in packaging material suitable for sterilization and storage. e.g. paper/plastic composite packaging.
7. Sterilize the adapter [→ 37].



7.4 Manual maintenance

7.4.1 Maintenance of mechanical parts

Intervals

- Prior to each sterilization
- After every thermal disinfection without integrated maintenance


Required accessories

- A Spray adapter
- B O-ring for spray adapter
- C T1 Spray

NOTICE! Only use Sirona T1 spray.


Procedure

- ✓ The spray adapter is disinfected.





Operating Instructions ENDO 6:1

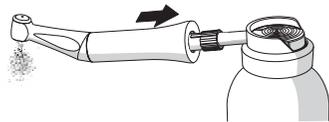


- ✓ The O-ring on the spray adapter is intact.
- 1. Fit the spray adapter onto the nozzle of the spray can.
- 2. Insert the instrument until it snaps into place and hold it.
- 3. Spray the instrument for 1 - 2 seconds.
IMPORTANT: Hold the spray can upright.
- 4. Wipe any spray that comes out with a disinfection cloth.
- 5. Repeat the process until the spray is clear.

7.4.2 Care of the push button chuck

Use T1 spray on the push button chuck to remove deposits and ensure proper functioning of the clamping system.

Interval

- At least once a week




7 Conditioning





7 Conditioning

Operating Instructions ENDO 6:1




Required accessories

A	Black nozzle insert
B	T1 spray

NOTICE! Only use Sirona T1 spray.


Procedure


- ✓ The instrument is clean and disinfected.
- 1. Press the contra-angle handpiece head with the chuck firmly against the spray can nozzle.
- 2. Spray the chuck for 1 - 2 seconds.
IMPORTANT: Hold the spray can upright.
- 3. Wipe any spray that comes out with a disinfection cloth.

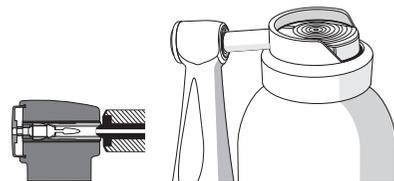


36

62 78 381 D3451.201.01.05.02






Operating Instructions ENDO 6:1






7.5 Sterilizing

- ✓ The instrument is clean and disinfected.
- ✓ Instrument maintenance is complete.
- ✓ If necessary, the instrument can be sterilized in packaging suitable for sterilization and storage, e.g. paper/plastic composite packaging or container.
- Sterilize the instrument in the steam sterilizer with saturated water vapor.

Overpressure: 2.04 bar (29.59 psi)
 Temperature: 134° C (274° F)
 Holding time: 3 min




7 Conditioning



62 78 381 D3451.201.01.05.02



37





7 Conditioning




Operating Instructions ENDO 6:1

Steam sterilizers that fulfill the requirements of either EN 13060, class B (for example, DAC PROFESSIONAL) or EN 13060, class S and are suitable for the sterilization of straight/contra-angle handpieces are approved.

NOTICE! Do not exceed 140°C (284°F), even during the drying phase.

After sterilizing

1. Remove the instrument from the steam sterilizer immediately.
⚠ CAUTION! The instrument is hot. Risk of burns!
NOTICE! Do **not** attempt to accelerate the cooling process by immersing the instrument in cold water. This can damage your instrument.
2. Store all instruments so that they are protected from contamination.
3. Sterilize again once the storage period has elapsed.






8 Spare parts and consumables

Use only original Sirona parts or parts approved by Sirona.

	REF		REF
T1 spray (6 x 250 ml cans)	59 01 665	Spray adapter (ISO) for spray can	89 17 858
O-ring for spray adapter	70 36 353	Insulating sleeve for Endo	63 24 631






9 Storage and transport conditions




Protect from moisture




Sensitive contents



Relative humidity




Air pressure



Temperature

After a severe change in temperature, allow sufficient time for acclimatization.






6278381.book Seite 41 Donnerstag, 12. Februar 2015 9:29 09



Operating Instructions ENDO 6:1



62 78 381 D3451.201.01.05.02




10 Disposal

- According to current information, the product does not contain any substances that are hazardous to the environment.
- Disinfect the product prior to disposal.
- Observe the applicable disposal regulations for your area.



10 Disposal



41





We reserve the right to make any alterations which may be required due to technical improvements.



D3451.201.01.05.02 12.2014

Ä.-Nr.: 116 169



Sirona Dental Systems GmbH
Fabrikstraße 31
D-64625 Bensheim
Germany www.sirona.com

in USA: Sirona Dental Systems, LLC
4835 Sirona Drive, Suite 100
Charlotte, NC 28273
USA www.sirona.com

62 78 381 D3451

